


## Tracking Shock Sensation Stimulator

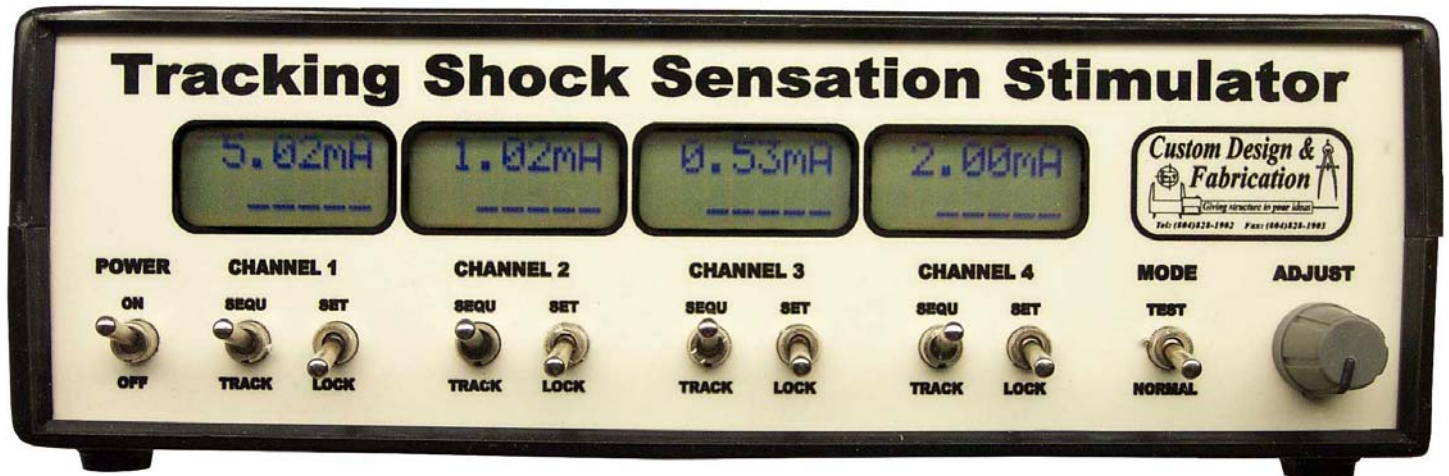

The **Tracking Shock Sensation Stimulator** is an effective tool for behavioral modification. The device utilizes an isolated and regulated alternating current source to provide a safe, yet effective, electrical stimulation, while sufficient source potential ensures consistent negative reinforcement conditioning for almost any subject. The level of discomfort is adjustable to obtain adequate deterrent value without being unnecessarily cruel or traumatic.

The stimulator provides four individually controlled output channels each with its own diagnostic bar graph for detecting electrical problems and monitoring the actual stimulus delivered. The diagnostic bar graph and precision current regulation ensure the electrical integrity of the system and eliminate inconsistencies experienced with similar products.

**For information or orders, contact:**

**Guy M. Blankinship III**  
Virginia Commonwealth University  
Medical Center  
1101 East Marshall Street, Room B1-060  
P.O. Box 980470  
Richmond, Virginia 23298-0470  
Phone: (804) 828-1902  
Fax: (804) 828-1903  
E-mail: [gblankin@vcu.edu](mailto:gblankin@vcu.edu)

